

BLUEMEDICAL

A Translumina Group Company



FORCE NC
NON-COMPLIANT

P r e c i s e p o w e r f u l
p o s t d i l a t a t i o n

FORCE NC


NON-COMPLIANT

PTCA NC Balloon Catheter

FORCE NC, the high pressure PTCA catheter that ensures pressure when pressure is needed without compromising on flexibility, profile and catheter performance.

Now get the catheter with superb performances that enables precise and safe post dilatation.

Excellent re-wrap and re-cross

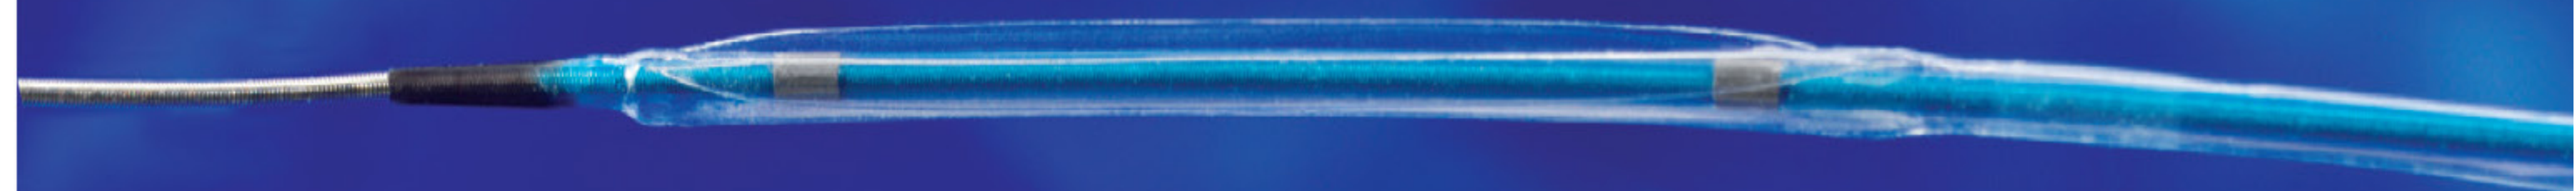

FORCE NC

NON-COMPLIANT

THE LOW PROFILE, FLEXIBLE HIGH PRESSURE PTCA

High rated burst pressure

- Rated burst pressure 21 bar (2,0-3,0 mm), nominal pressure 12 bar
- Providing an extensive and safe working range

Conformability

- No longitudinal growth for controlled expansion, even at high pressures
- No balloon deformations up to rated burst pressure for precise stent apposition
- No dog boning between nominal and rated burst pressure

Flexibility and low profile

- Optimized materials and design for flexibility and low profiles
- Ease of use equal to high performance workhorse catheters



PTCA CATHETER



Real non compliant

- Real non compliant: ~1% growth per atmosphere between nominal and rated burst pressure
- Controlled equal growth during inflation up to rated burst pressure
- Precise compliance ensuring exact and protected sizing

Hydrophilic coating

- Fully coated, tip to distal shaft including folded balloon
- Reduced likelihood of catheter friction enhances ease of passage
- Remains durable during multiple inflations

BALLOON CATHETER COMPLIANCE CHART

Pressure (bar)	Ø2.00 (mm)	Ø2.50 (mm)	Ø2.75 (mm)	Ø3.00 (mm)	Ø3.25 (mm)	Ø3.50 (mm)	Ø4.00 (mm)	Ø4.50 (mm)
4	1.74	2.27	2.46	2.75	2.83	3.13	3.57	4.07
5	1.78	2.31	2.48	2.80	2.86	3.16	3.65	4.15
6	1.82	2.35	2.51	2.84	2.91	3.23	3.73	4.23
7	1.85	2.38	2.55	2.87	2.96	3.30	3.80	4.30
8	1.90	2.41	2.60	2.90	3.01	3.35	3.86	4.36
9	1.93	2.44	2.65	2.93	3.08	3.40	3.91	4.41
10	1.96	2.46	2.68	2.96	3.13	3.44	3.95	4.45
11	1.98	2.48	2.72	2.98	3.18	3.47	3.98	4.48
12 NP	2.00	2.50	2.75	3.00	3.25	3.50	4.00	4.50
13	2.03	2.52	2.77	3.02	3.27	3.52	4.03	4.53
14	2.06	2.54	2.79	3.04	3.30	3.55	4.06	4.56
15	2.09	2.56	2.82	3.06	3.33	3.58	4.08	4.58
16	2.11	2.58	2.84	3.08	3.37	3.60	4.11	4.61
17	2.14	2.60	2.86	3.11	3.41	3.63	4.14	4.64
18	2.16	2.62	2.89	3.13	3.44	3.66	4.17	4.67
19 RBP	2.18	2.64	2.91	3.15	3.48	3.68	4.20	4.70
20	2.21	2.66	2.93	3.18	3.50	3.71	4.23	4.73
21 RBP	2.24	2.69	2.96	3.20	3.54	3.74	4.26	4.76
22	2.27	2.71	2.99	3.23	3.58	3.77	4.32	4.82
23	2.30	2.74	3.02	3.25	3.61	3.81	4.35	4.85
24	2.33	2.76	3.05	3.30	3.64	3.85	4.39	4.89
25	2.36	2.79	3.08	3.34	3.68	3.89	4.45	4.95
26	2.40	2.82	3.11	3.38	3.71	3.95	4.51	5.01

1 bar = 100 kPa

NP: Nominal Pressure RBP: Rated Burst Pressure. Do not exceed

FORCE NC

NON-COMPLIANT

TECHNICAL DATA

FORCE NC
NON-COMPLIANT

Nominal Pressure:	12 bar
Rated Burst Pressure:	Ø 2.00 - 3.00 = 21 bar Ø 3.25 - 4.50 = 19 bar
Balloon material:	Non-compliant polyamide for controlled dimensions
Folding:	3-folds
Guiding catheter compatibility:	5F (min ID 0.056"/1.42 mm)
Guide wire compatibility:	max 0.014" (0.36 mm)
Catheter type:	Rapid Exchange
Proximal shaft:	1.9F (0.64 mm)
Distal shaft:	2.7F (0.90 mm)
Tip entry profile:	0.016" (0.40 mm)
Usable Catheter Length:	154 cm
Tapered tip:	3.5 mm
Shaft coating:	Hydrophilic coating
Shelf life:	3 Years from sterilization date

FORCE NC

NON-COMPLIANT

ORDER NUMBERS


Diameter (mm)

L \ Ø	Diameter (mm)							
	2.00	2.50	2.75	3.00	3.25	3.50	4.00	4.50
5*	XFOR2005	XFOR2505	XFOR2705	XFOR3005	XFOR3205	XFOR3505	XFOR4005	XFOR4505
10	XFOR2010	XFOR2510	XFOR2710	XFOR3010	XFOR3210	XFOR3510	XFOR4010	XFOR4510
15	XFOR2015	XFOR2515	XFOR2715	XFOR3015	XFOR3215	XFOR3515	XFOR4015	XFOR4515
20	XFOR2020	XFOR2520	XFOR2720	XFOR3020	XFOR3220	XFOR3520	XFOR4020	XFOR4520

Length (mm)

Order number description: XFOR DDLL (D=Diameter, L=Length)

* L: 5 mm has only one marker

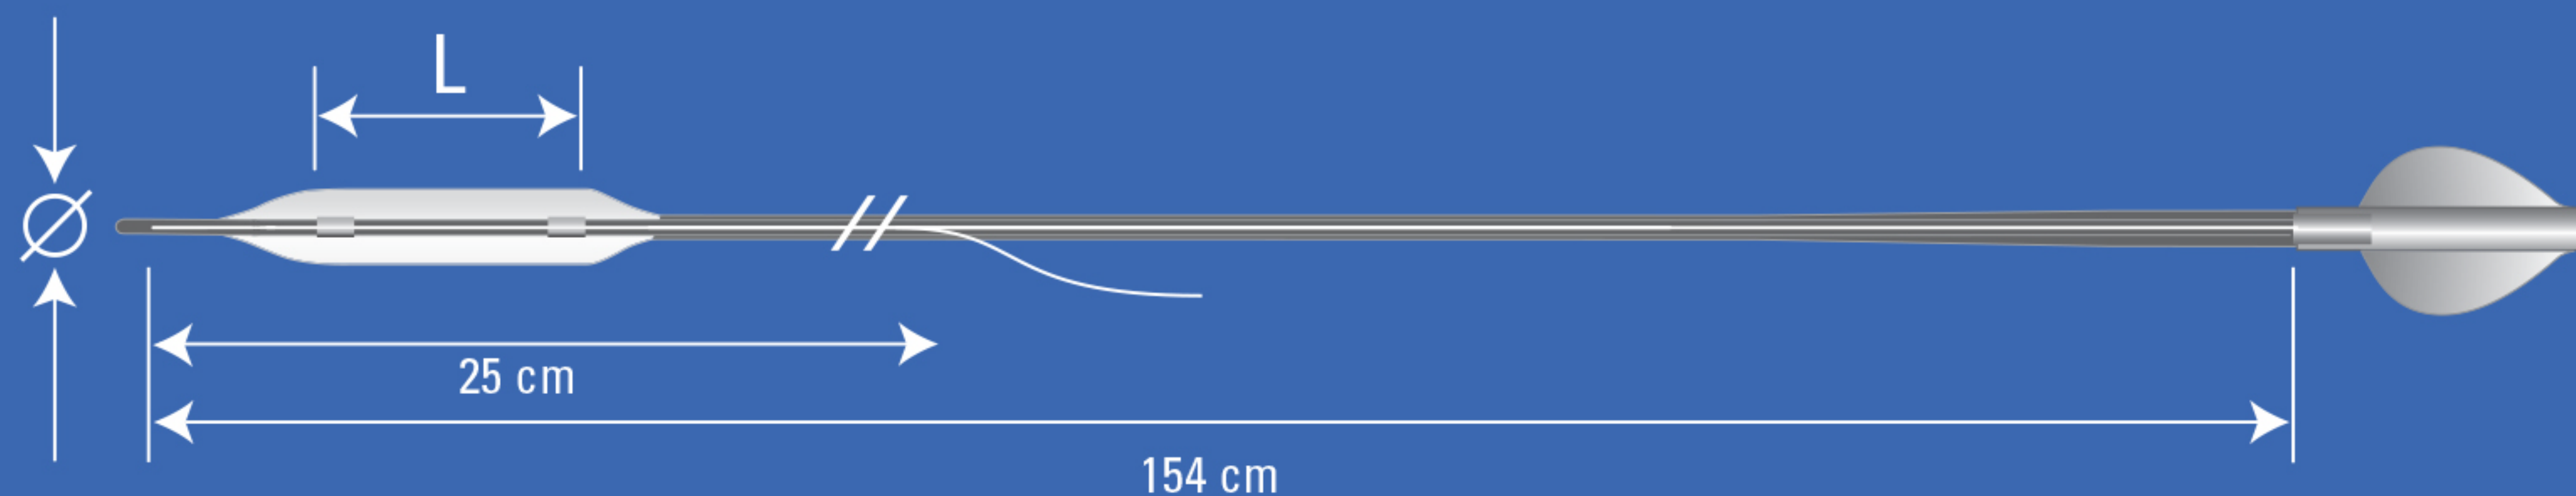**BLUEMEDICAL**

A Translumina Group Company

BLUE MEDICAL DEVICES B.V., PANOVENWEG 7, 5708 HR HELMOND, THE NETHERLANDS
 PHONE: +31 (0)850 073 000, E-MAIL: sales@welling.com, WWW.WELLINQ.COM

Indications, contraindications, warnings and instruction for use can be found in the product labeling.
 CAUTION: restricted to sale by or on the order of a physician

XFO9.0001.11 01/23